



PROFICIENCY TESTING
SYSTEMS

PROGRAM 2021 /
PROGRAM PREVIEW 2022



...quality assured

Proficiency Testing Systems In Quality Assurance

Program 2021 / Program Preview 2022

Test the reliability of your analyses!

❖ **Chemistry** ❖ **Microbiology** ❖ **Sensory**

Proficiency testing systems are an efficient instrument for internal and external quality assurance. Concerning accreditation and certification bodies, proficiency tests are a significant tool to demonstrate the analytical performance of the own laboratory. At a glance there is a plenty of information regarding the effectiveness and accuracy of the used method and the competence of the personal equipment. Furthermore the failures or tendencies in analysis can be recognized and corrected to guarantee the analytical performance on a constant high level. Confidential results avoid expensive charges and lead to high economic efficiency. Finally you are able to enhance the business confidence and the reliability of the certification authorities.

The **proficiency testing program** for quality assurance of MUVA KEMPTEN GMBH is one of the worldwide most important schemes for chemical, microbiology and sensory analysis of food. Since 25 years, MUVA KEMPTEN GMBH has experience in performing proficiency testing studies and in the applied statistics. MUVA KEMPTEN GMBH cooperates with a number of national and international working groups and is - since a long time - close with quality management and analytical quality assurance.

The whole expert knowledge of the MUVA KEMPTEN GMBH is available to our proficiency testing team and as a matter of course our clients can access it at any time.

muva kempten GmbH
Your accredited international provider for proficiency testing schemes in food analysis

FROM OUR PROFICIENCY TESTING PROGRAM YOU CAN EXPECT


- ❖ a precise and reliable planning and organization which complies with recognized international standards like the new standard DIN EN ISO/IEC 17043:2010-05 and ISO 13528:2015 as well as the International Harmonized Protocol for Proficiency Testing of (Chemical) Analytical Laboratories
- ❖ a neutral and strictly confidential treatment and presentation (encoded) of your results
- ❖ a detailed report with a traceable and understandable evaluation, together with clear graphical and tabular presentations and recommendations as well as helpful suggestions
- ❖ a certificate which presents your own z- and z' - scores, well-arranged
- ❖ a good value for money

PROFIT FROM A CONTINUOUS PARTICIPATION IN PT BY OFFER "EVALUATION OF YOUR PERFORMANCE DEVELOPMENT"

By means of the graphical evaluation of your analytical performance

- ❖ the competence of the laboratory is presented excellently and can so be documented to third parties in an easy way
- ❖ Tendencies and systematic failures (bias) become apparent at a glance
- ❖ The competence of e.g. your technicians, different devices etc. can be tracked over a longer period

Example: Performance Development as Shewhart Control Chart

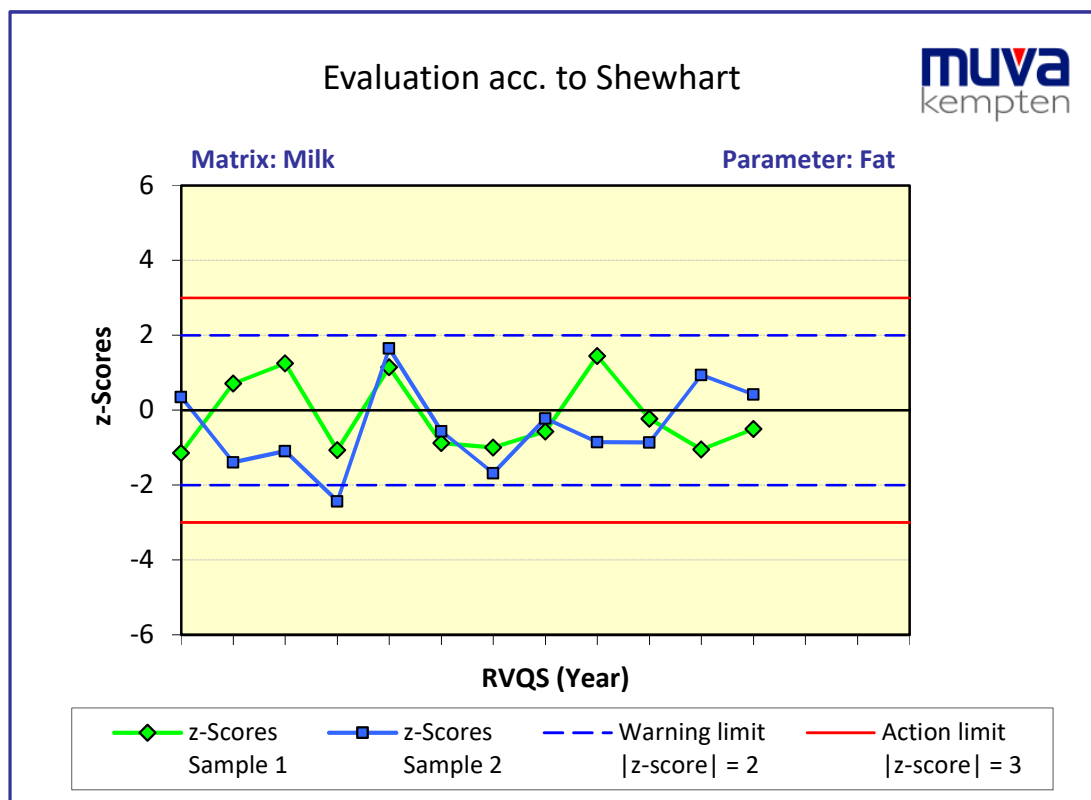

Please regard our registration form on the homepage: www.muva.de → [proficiency testing!](#)

- ❖ Set up an account in our comfortable online portal
- ❖ Two weeks at the latest before sample shipment, you receive the study announcement together with the relevant target dates (dispatch of the samples, deadline for results). You can download all supporting documents, which will be available on the online portal in time. If you require additional sample material, please inform us immediately via an informal e-mail. It is possible to cancel the registration within one calendar week after receiving the announcement of the present proficiency test. We feel free to charge the costs incurred. After the above-mentioned dead line, we will invoice the total costs of the proficiency testing study.
- ❖ We will inform you about the sample shipment in a separate e-mail. As announced, you will receive two samples, which are tested for homogeneity and stability, equal in composition, but with different contents in selected parameters. It is on your choice if you will analyse all or some of the provided parameters. Ideally, you will analyse each parameter in duplicate with the method of your choice. Further duplicate determinations are possible (e.g. using another method, on a different day or by different technicians). Please report the results until the fixed target date (usually within 3 weeks).
- ❖ The submission of results is possible in the online portal – both simply and conveniently. Results for one or both samples and for the parameters of your choice can be entered and either transmitted collected or one by one. More detailed information on using our online portal are available at [www.muva.de / proficiency testing](http://www.muva.de/proficiency_testing)
- ❖ Within 1 - 2 months, the report (with all information encoded) will be accessible in the online portal. Additionally downloading is possible. You will receive the certificate and the invoice by post, unless otherwise agreed.
- ❖ The report contains the following information
 - ◆ the number of participating laboratories
 - ◆ the used methods
 - ◆ all data of homogeneity
 - ◆ the summary of results
 - ◆ recommendations and the annex

In the annex, you find the tables with

- ◆ all single and mean values
- ◆ the corresponding methods with all relevant information
- ◆ the performance criteria z-score and z'-score
- ◆ the estimated, extended measurement uncertainty for the laboratory that provided three or more results for a method
- ◆ statistical data (extensive information on the statistical evaluation you may find in our statistical protocol under [www.muva.de / proficiency testing](http://www.muva.de/proficiency_testing))

as well as graphical presentations (see examples on the following page).

- ❖ After the study, we are glad to be at your command for questions and recommendations. In between the studies and in case of disappointing results we recommend using the reference materials of MUVA KEMPTEN GMBH.
- ❖ The proficiency tests in chemical and microbiological studies take place, starting by a number of ten laboratories. The sensory proficiency testing studies take will proceed with more than five participating laboratories, due to the fact that each panel participate with several panellists. In average, the number of participants is usually about 35 participants per proficiency test. The participation is possible for laboratories of all scientific fields and not limited to special topics.
- ❖ Amongst others laboratories of food research and testing institutes, food testing laboratories, private laboratories, as well as food, veterinary and costumes inspection services participate in the proficiency testing studies of MUVA KEMPTEN GMBH.

CALCULATION OF THE METHOD DEPENDING MEASUREMENT UNCERTAINTY BASED ON THE NORTH TEST

Starting at 3 results provided by a laboratory (in chemical proficiency testing schemes at minimum 6 single results) using one method for analysis, the contributions of the uncertainty are determined from the standard deviation calculated on basis of the single results (= reproducibility) and the bias of the single results in relation to the assigned value. The extended measurement uncertainties are assessed on basis of the North Test and they are listed in the evaluation tables of each parameter. If a laboratory provided sufficient results for more than one method, the measurement uncertainties are estimated and listed separately for each method.

These measurement uncertainties are for information only but they can be an excellent tool for the plausibility check of the own estimated measurement uncertainty. It is not suitable to use it as generally valid measurement uncertainty for subsequent results in routine analysis.

Example: Extract of an evaluation table with extended measurement uncertainty of a laboratory


Tab. 1: Ergebnisse in Probe 1 Table 1: Results of sample 1							Zugewiesener Wert ± Unsicherheit Assigned value ± uncertainty		1,58 ± 0,04 (g/100g) (g/100g)	
Lab Code	X _{lab} Wert 1 Value 1 (g/100g)	X _{lab} Wert 2 Value 2 (g/100g)	X _{lab} Mittelw. Mean (g/100g)	Meth. Code	Methode / Method Beschreibung Description		Kommentar Comment	Bewertung Performance		Mess- sicherheit / measurement uncertainty U _{lab}
	Norm (Standard) Standard	z-Score	z'-Score							
1,1	1,51	1,47	1,49	b52	102 °C	VDLUFA C 35.9		-1,02	-0,69	
1,2	1,42	1,47	1,45	b52	102 °C	VDLUFA C 35.9		-1,53	-1,04	
2	keine Ergebnisse / no results									
3	1,58	1,54	1,56		102 °C	ÖNORM EN ISO 3727-1		-0,23	-0,15	
4	1,64	1,66	1,65		102 °C		int. Meth.	0,80	0,54	
5,1	1,58	1,64	1,61	b52	102 °C	VDLUFA C 35.9		0,34	0,23	0,20
5,2	1,55	1,54	1,55	b52	102 °C	VDLUFA C 35.9		-0,40	-0,27	
5,3	1,47	1,46	1,47	b52	102 °C	VDLUFA C 35.9		-1,31	-0,89	
6	1,50	1,57	1,54	b53	102 °C	VDLUFA C 35.10		-0,51	-0,35	

GRAPHICAL PRESENTATION OF THE PROFICIENCY TESTING RESULTS

The different graphical representations allow a quick overview on all data. Furthermore, it is possible to gain additional information.


The following figure shows the data sorted by ascending values. This graph also presents the warning and action limits of the corresponding evaluation criteria. Thus, the distribution with regard to the evaluation criteria are visible at a glance.

Example: Evaluation of the results sorted by size with limits of the evaluation criterion z-score (fat content in cream cheese)

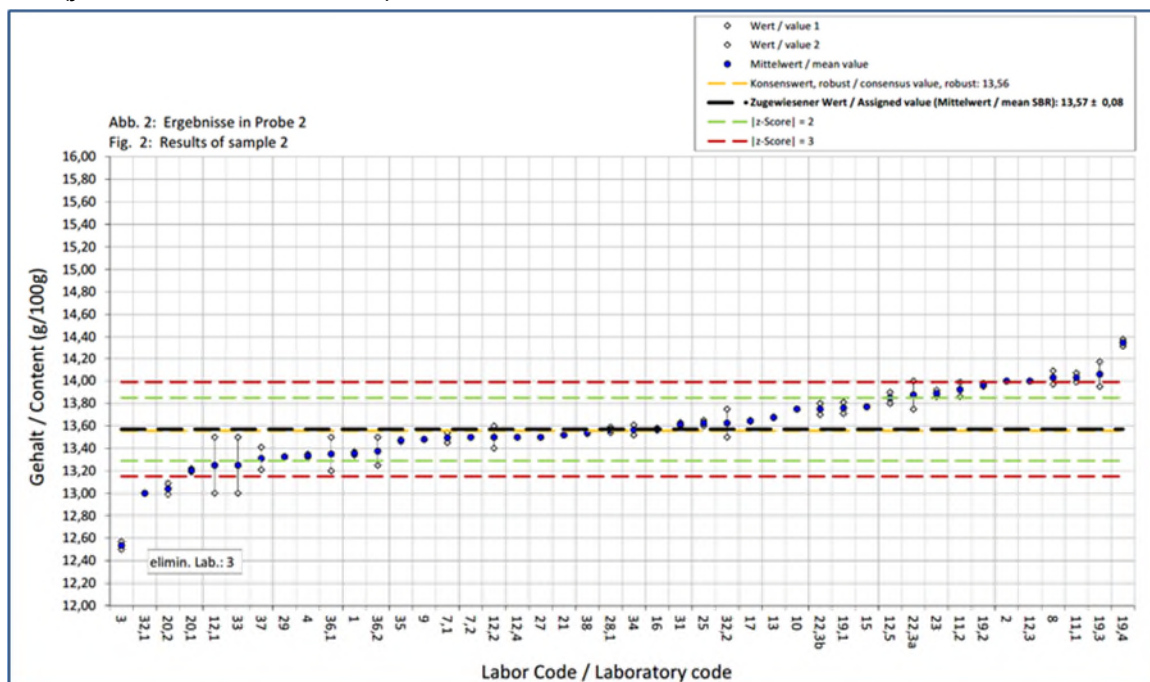


The figure “evaluation of the results according to the methods” allows the assessment of the efficiency of the different methods. Moreover, the participants are able to compare their own results with those of the other laboratories within the methods as well as between the methods.

Example: Evaluation of the results according to the methods (fat content in cream)

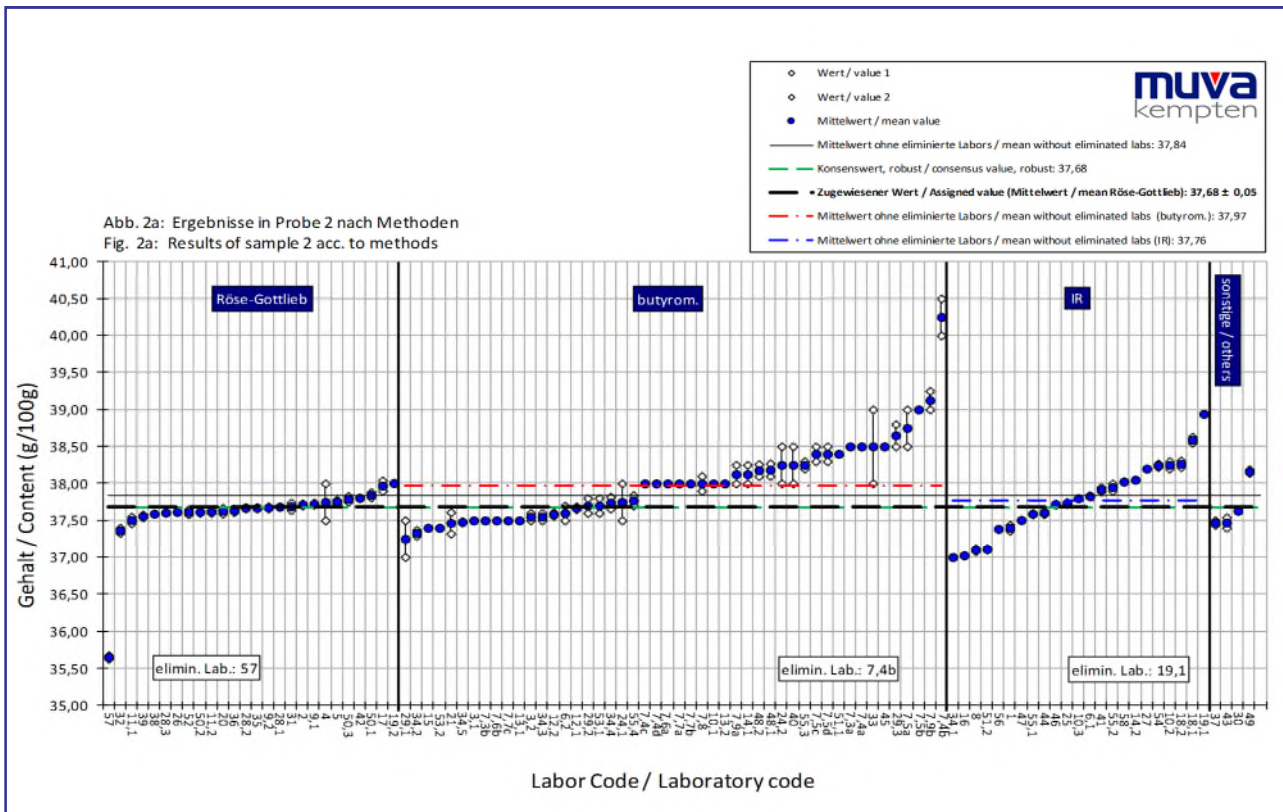


The figure of z-scores shows the performance of the participants at a glance. Additionally the laboratories are able to detect systematic errors (e.g. if the z-scores in both samples are >3).

Example: Colored figure of z-scores for dry matter in milk powder

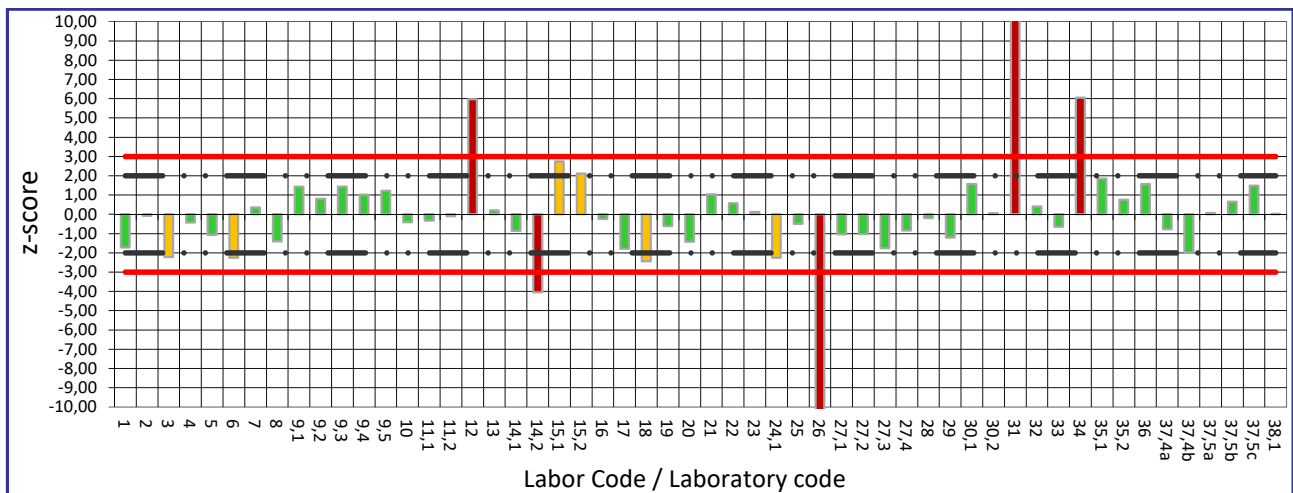

The Youden-Plot demonstrates very clearly, when a method is affected by a systematic error.

Example: Youden-Plot, fat content in two cream samples, view for tendencies

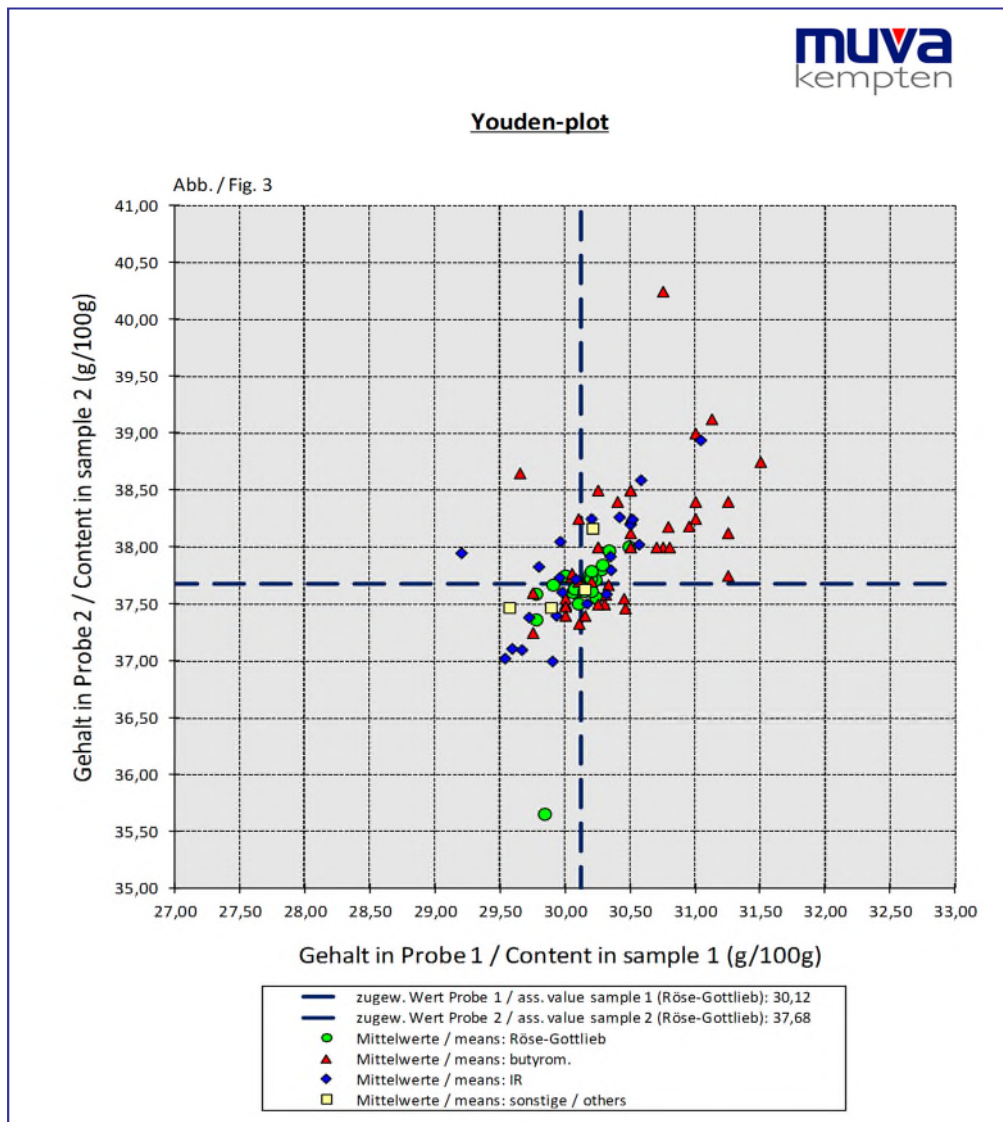

INNOVATIVE SENSORY PROFICIENCY TESTING SYSTEM

DESCRIPTION OF THE SENSORY PROFICIENCY SYSTEM FOR FOOD INDUSTRY



Assure the quality of your senses!


❖ **Odour** ❖ **Taste** ❖ **Touch** ❖ **Sight** ❖ **Hearing**

Research and development in sensory proficiency testing schemes support the assurance for quality at sensory working. Sensory panels have the possibility to compare their performances with other panels. Moreover the assessment of the individual panellist among each other is very important for the quality assurance, too. It can be an excellent instrument to select and supervise sensory panels. Our Sensory Proficiency Testing System consists of different tests used in the daily routine work and the offer of four senses – odour, taste, touch and sight. So the validation of the quality and performance of your panel and panellists can be enabled.

PERFORMANCE DEVELOPMENT

On the subject of the evaluation of the sensory proficiency testing studies “rank order”, MUVA KEMPTEN GMBH developed a new point system for the assessment of the panellists’ performance. According to the page test and regarding the identification of the correct basic taste or odour points between 0 and 10 are assigned. The top of the score 10 is given for the correct rank order and the correct identification of the basic taste. For sensory analyzing the identification of the correct basic taste as well as the correct aroma is very important, so if there is a failure in the identification the points are divided of two. With the aid of this point system a continuous monitoring of quality is possible; for example by the use of control charts.

Example: Performance card of continuous participation in proficiency testing studies

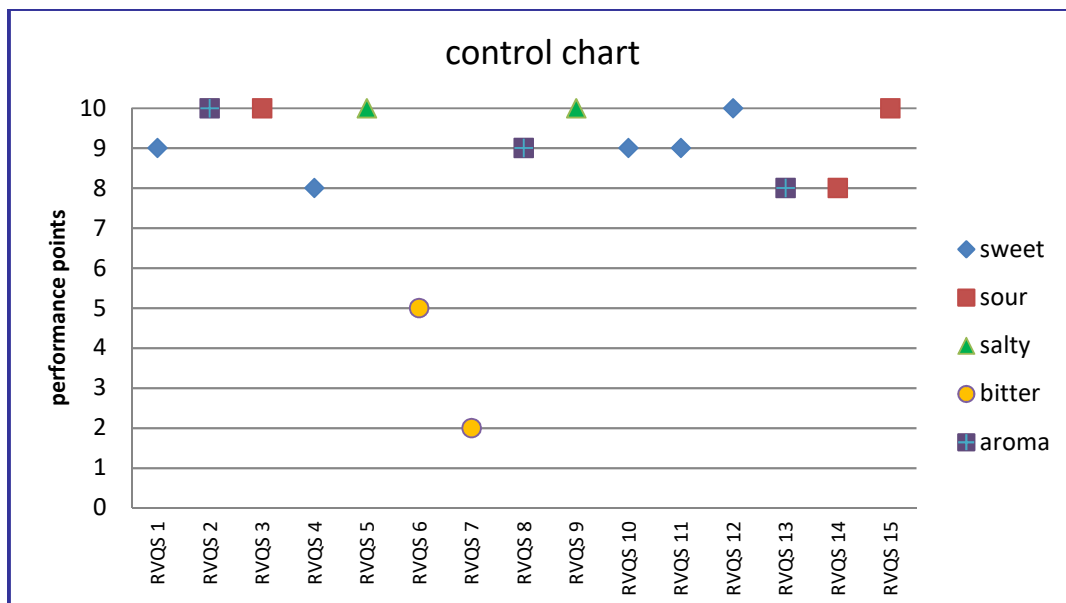

The composition and process of the sensory PT’s are equivalent to the chemical and microbiological PT’s.

<p>RANK ORDER</p> <p>Identification of the test criteria in taste (basic tastes) or odour (aroma) and ranking test according DIN ISO 8587 with 4 analyzing samples.</p>
<p>PROFILE TESTING</p> <p>Profiling of an analyzing sample by two reference samples in at least 5 attributes.</p>
<p>TRIANGLE TEST</p> <p>Evaluation of the level of significance of the panellists and panels according DIN 4120 by testing 6 sets of triangle tests.</p>
<p>PACKAGING MATERIAL</p> <p>Intensity test in odour and taste of a utensil according to DIN 10955 and a triangle test.</p>
<p>FATS AND OILS</p> <p>The analyzing of “virgin, cold-pressed rapeseed oil” and “frying fat” according to characteristic and dissimilar attributes given in the German Method “DGF Einheitsmethode C-II 1” (DGF = German society of fat science).</p>
<p>TESTING ACC. TO DIN EN ISO 22935</p> <p>Evaluation of milk and dairy products according to the 5-point-scale of DIN EN ISO 22935.</p>
<p>ODOUR THRESHOLD VALUE (TON) AND TASTE THRESHOLD VALUE (TFN)</p> <p>Determination of the odour threshold value (TON) and the taste threshold value (TFN) in drinking water by the use of a comparison of pairs according to DIN EN 1622.</p>


For comparability at a glance, all results are listed encoded in tables and graphics. See the examples at point “graphical presentation of the results”. In all proficiency testing studies the interesting statistical values – for example mean, median, standard deviation etc. – are calculated. In the reports there is also statement about the qualification for sensory measurements for each panel and each assessor.

ASSURANCE OF THE MATERIAL


The material is tested of homogeneity to ensure the sensory properties. The homogeneity test is equivalent with corresponding chemical analyses according to BCR/48/93. Sensory experts of MUVA KEMPTEN GMBH organize the sensory measurements. The verification of the material occurs consecutively monitoring by the performance of the proficiency testing and the chemical and microbiological quality assurance.

EN ISO 4120; 8.2 is used to ensure the homogeneity and similarity of the analyzing material for the triangle test. The results are evaluated according to table A.2 of EN ISO 4120.

Example for a graphic presentation: Identification of the correct aroma in a circle diagram.

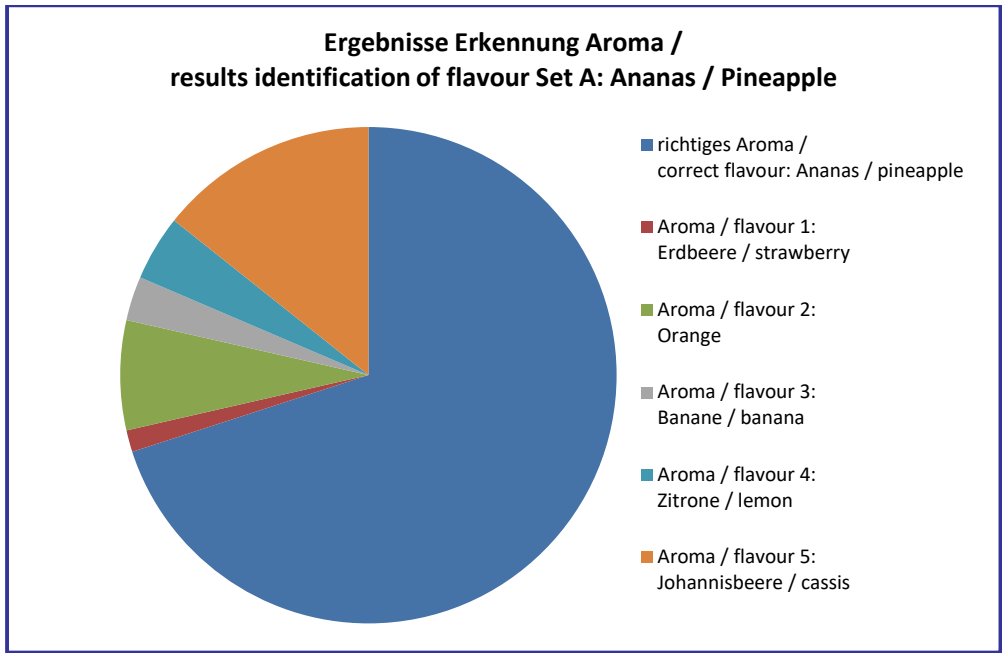

Example for a graphic presentation: Results in profile testing by using a spider web.

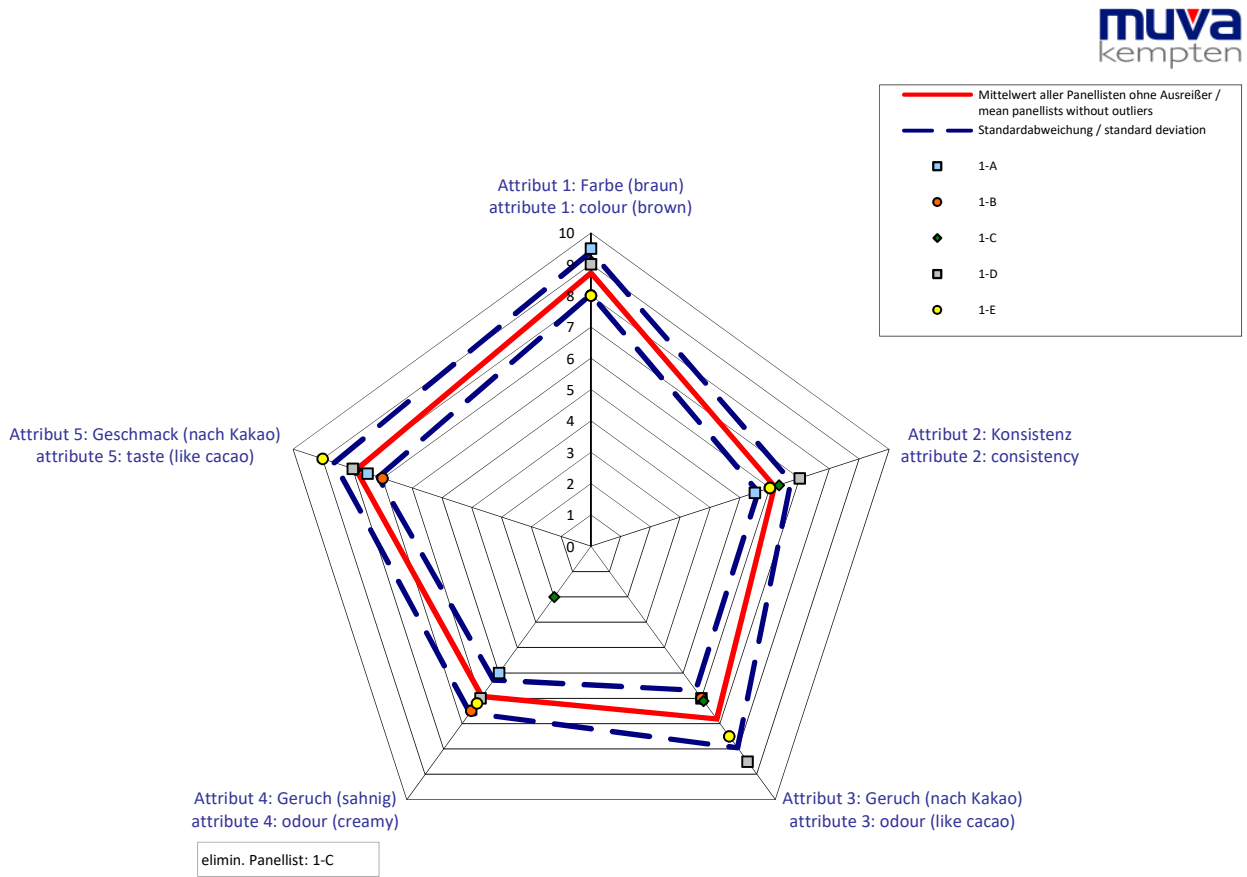

REFERENCE MATERIAL

After participation in proficiency testing studies of MUVA KEMPTEN GMBH, you have the opportunity to buy the material used in this muva proficiency testing study.

We recommend using our muva reference material in the meantime of the proficiency studies for a regular (statistical) quality control of your own panel and each individual assessor.

WORKSHOP AND INHOUSE-TRAINING

Every year, the department of proficiency tests and reference materials of MUVA KEMPTEN GMBH offers minimum one workshop dealing with quality assurance and / or statistics in quality assurance.

Additional we are glad to visit your company for special training dealing with subjects of your own choice.

Please contact us.

REBATE SYSTEM FOR PROFICIENCY TESTING IN CHEMISTRY AND MICROBIOLOGY

The rebate for the proficiency testing studies in chemistry and microbiology is based on the transaction volume of the customer in proficiency testing / reference material of the previous year. The discount is as follows:

- *from 5.000,- €: 5% rebate*
- *from 10.000,- €: 10% rebate*
- *from 15.000,- €: 15% rebate*
- *from 20.000,- €: 20% rebate*

REBATE SYSTEM FOR PROFICIENCY TESTING IN SENSORY

The discount for the proficiency testing studies in sensory depends on the number of panellists as follows:

- *3 – 5 persons (incl. panel evaluation) 5% rebate*
- *6 – 9 persons (incl. panel evaluation) 10% rebate*
- *≥ 10 persons (incl. panel evaluation) 15% rebate*

SHIPPING CONDITIONS

The dispatch of the sample materials for the proficiency testing studies is ex works.

Packing and shipping costs will be charged according to the expenses. Do not hesitate to contact us for more information.

REGISTRATION TERMS

There is the possibility to select a subscription or to register yearly. We ask for your understanding for the following arrangement. Please note that we need your registration for your participation in proficiency testing studies performed in January 2021 at the latest by the end of November 2020.

Please note the valid [general terms of business](#) as well as the [privacy statement](#) drawn up by muva kempten GmbH (www.muva.de).

PROGRAM PROFICIENCY TESTING STUDIES 2021 / 2022

PLEASE NOTE, THE REGISTRATION WILL TAKE PLACE IN OUR COMFORTABLE ONLINE PORTAL

- If you do not have an access yet, please register as a customer first: <https://service.muva.de>
- For the efficient use of the portal, we provide **instructions** for registration, booking PTs and submission of results on our [homepage](#).
- If you would like to order a **subscription**, we kindly ask you to register your proficiency tests by the online portal once and click on the option "book as a subscription".
- Please indicate in the field „message“ when booking, if you need **additional sample materials** or for specifying the **number of panellists**. If this is unknown yet, you can send us an informal e-mail at any time before shipment of the samples.
- For an additional charge of € 9.00 you can still receive the **results report** in **paper form**. If applicable, please indicate this also in the field " message ".
- Please note that our program is now **designed for two years**. Additionally, in the future **some proficiency tests** will take place alternatingly **every two years**.
- **You can book the tests for the year 2022 from autumn 2021**. The prices are valid for the current year.
- **We reserve the right to make any changes if necessary**. In such cases we will inform you in time as a matter of course.

Please contact us for any questions, we are glad to support you!

**MUVA KEMPTEN GMBH –
your accredited international provider for proficiency tests in food analysis**

Type	Product	EPQS	2021	scheduled in 2022	Parameter	Price ¹⁾	
						Report PDF	add. result ²⁾
CHEMISTRY							
MILK							
A	Milk	873	Jan	Jan	Fat, Dry Matter, Protein, Lactose (monohydrate), Freezing Point, Density	225 €	78 €
A	Milk	896	May	May	Fat, Dry Matter, Protein, Lactose (monohydrate), Freezing Point, Calcium	225 €	78 €
A	Milk	911	Sep	Sep	Fat, Dry Matter, Protein, Lactose (monohydrate), Freezing Point, pH Value	225 €	78 €
AL	Milk (low in lactose/lactose free)	880	Feb	Feb	Lactose (monohydrate), Galactose, Glucose	139 €	49 €
K	Raw Milk shock frozen	884	Mar	Mar	Fat, Dry Matter, Protein, Lactose (monohydrate), Freezing Point, pH Value, Casein	270 €	90 €
K	Raw Milk shock frozen	918	Oct	Oct	Fat, Dry Matter, Protein, Lactose (monohydrate), Freezing Point, pH Value, Urea	270 €	90 €
DAIRY PRODUCTS							
D	Cream	877	Jan	Jan	Fat, Dry Matter, Protein	159 €	55 €
D	Cream	909	Aug	Aug	Fat, Dry Matter, Protein	159 €	55 €
E	Evaporated milk / Coffee cream	898	May	May	Fat, Dry Matter, Protein, Phosphorus, Ash	209 €	75 €
H	Butter	881	Feb	Feb	Water, Solid non-fat, pH Value, Cholesterol, Butyric Acid Methyl Ester, Chloride, Sodium (sodium chloride)	189 €	70 €
L	Yoghurt	882	Feb	Feb	Fat, Dry Matter, Protein, Total Lactic Acid, pH Value	199 €	75 €
CHEESE							
C	Processed cheese	885	Mar	Feb	Fat, Dry Matter, Protein, Lactose (monohydrate), pH Value, Citric Acid, Ash, Chloride, Sodium (sodium chloride)	265 €	95 €
C	Processed cheese	908	Aug	Aug	Fat, Dry Matter, Protein, pH Value, Phosphorus, Ash, Chloride, Sodium (sodium chloride)	265 €	95 €
F	Cream cheese	893	Apr	Apr	Fat, Dry Matter, Protein, Lactose (monohydrate), pH Value, Total Lactic Acid, Chloride, Sodium (sodium chloride)	179 €	69 €
V	Cheese (hard / semi-hard cheese)	875	Jan	Jan	Fat, Dry Matter, Protein, pH Value, Chloride, Sodium (sodium chloride)	190 €	69 €
POWDER							
B	Milk powder	878	Feb	Jan	Fat, Free Fat, Dry Matter, Protein, Lactose (monohydrate), Ash	245 €	87 €
B	Milk powder	906	Aug	Aug	Fat, Dry Matter, Protein, Lactose (monohydrate), pH value, Ash	245 €	87 €
G	Whey powder	891	Apr	Apr	Fat, Dry Matter, Protein, Lactose (monohydrate), Calcium, Magnesium, Nitrate, NPN, Ash, Total Lactic Acid	289 €	115 €
P	Whey protein concentrate/ Sodium caseinate	900	Jun	Jun	Fat, Water, Protein, Lactose (monohydrate), Ash	215 €	80 €
T	Carbohydrates / Vitamins (in baby foods)	/	/	Apr	Glucose, Fructose, Lactose (monohydrate), Saccharose, Vitamin A, Vitamin C, Vitamin E	219 €	80 €
U	Minerals / Trace Elements (in baby foods)	903	Jun	Jun	Sodium, Potassium, Calcium, Magnesium, Iron, Zinc, Copper, Manganese, Phosphorus, Chloride	298 €	129 €

Type	Product	EPQS	2021	scheduled in 2022	Parameter	Price ¹⁾	
						Report PDF	add. result ²⁾
OTHERS							
VP	Alkaline Phosphatase in Milk and Cheese	874	Jan	Jan	Phosphatase Activity; qualitatively + quantitatively	154 €	50 €
AM	Aflatoxin M1 in Milk	919	Oct	Oct	Aflatoxin M1	160 €	55 €
FS	Fruit Juice	922	Nov	/	Glucose, Fructose, Titratable Acid, Soluble Solids (*Brix), Ethanol, pH value, Patulin	179 €	65 €
S	Canned Sausage	901	Jun	/	Fat, Water, Protein, Hydroxyproline, Ash, Chloride, Sodium (sodium chloride)	179 €	65 €
FM	Fatty Acid Distribution in Milk Powder	921	Oct	Oct	C4 to C20; (C14:1, C16:1, C18:1, C18:1-trans, C18:2, C18:2-trans, C18:3)	223 €	75 €
N	Chocolate / Nougat	894	Apr	/	Fat, Milk Fat, Dry Matter, Protein, Lactose (monohydrate), Saccharose, Theobromine	199 €	70 €
HST1	Veterinary Drugs in Milk	924	Nov	/	Possible groups of substances: β -Lactam, Tetracycline, Sulfonamide, Cephalosporine, Quinolones; quantitative	245 €	89 €
HST2	Veterinary Drugs in Milk	925	Nov	Oct	Possible groups of substances: β -Lactam, Tetracycline, Sulfonamide, Cephalosporine; qualitative	165 €	59 €
MICROBIOLOGY							
OEE	E. coli / Enterobacteriaceae	923	Nov	Nov	E. coli, Enterobacteriaceae in frozen Milk	199 € ³⁾	55 €
OK	Mesophilic, Aerobic Bacterial Count	905	Jul	Jun	Total Bacterial Count (in Powder and freeze dried Cheese)	199 € ³⁾	55 €
OH	Yeasts	/	/	Feb	Yeasts (Capsules in Milk Products)	199 € ³⁾	55 €
OK	Mesophilic, Aerobic Bacterial Count	887	Mar	Mar	Total Bacterial Count in frozen Milk	199 € ³⁾	55 €
OEC	E. coli / Coliforme / Enterobacteriaceae	888	Mar	Mar	E. coli, Enterobacteriaceae, Coliforme in frozen Milk	199 € ³⁾	55 €
OHS	Yeasts / Moulds	889	Mar	Mar	Yeasts, Geotrichum in frozen Milk	199 € ³⁾	55 €
OK	Mesophilic, Aerobic Bacterial Count	913	Sep	Sep	Total Bacterial Count in frozen Milk	199 € ³⁾	55 €
OEC	E. coli / Coliforms / Enterobacteriaceae	914	Sep	Sep	E. coli, Enterobacteriaceae, Coliforms in frozen Milk	199 € ³⁾	55 €
OHS	Yeasts / Moulds	915	Sep	Sep	Yeasts, Geotrichum in frozen Milk	199 € ³⁾	55 €
OST	Staphylococcus	916	Sep	Sep	Staphylococcus in frozen Milk	199 € ³⁾	55 €

Basically, all testing samples of chemical and microbiological proficiency testing schemes are unfit for consumption!

¹⁾ Net price plus packing and shipping costs (will be charged according to the expenses)

²⁾ Additional double determination (results) and/or additional material

³⁾ The basic price includes up to **9 results**, each additional result is charged separately. If you participate twice (in spring and autumn) in the same proficiency test, you will receive a 15% discount for the second participation. **All sample materials contains strains of safety group S1.**

Type	Product	EPQS	2021	scheduled in 2022	Parameter	Price ⁴⁾	
						Report PDF	add. result ²⁾
SENSORY							
TASTE –SENSORY							
Se1	Rank Order	876	Jan	Jan	2 Sets of Basic Taste	239 € ⁵⁾	92 €
Se2	Rank Order	897	May	May	2 Sets of Basic Taste Fruit Juice and Liquid	239 € ⁵⁾	92 €
Se3	Rank Order	910	Aug	Aug	2 Sets of Basic Taste	239 € ⁵⁾	92 €
Se4	Rank Order	920	Oct	/	1 Set of Flavour	185 € ⁵⁾	85 €
SeRF	Rank Order in Sausage	895	May	May	Taste in Sausage	169 € ⁵⁾	79 €
SeP	Profile Testing	890	Mar	Mar	5 Attributes	352 € ⁴⁾	80 €
SeV	Packaging Material	917	Sep	Sep	Intensity test with triangle test for taste and odour	352 € ⁴⁾	105 €
SeD	Triangle Test	892	Apr	Apr	Taste	175 € ⁵⁾	79 €
SeDW	Triangle Test in Sausage	904	Jun	Jun	Taste in Sausage	185 € ⁵⁾	85 €
ODOUR-SENSORY							
SeA	Rank Order	/	/	Feb	Aromatic Solutions	169 € ⁵⁾	79 €
SeDA	Triangle Test	883	Feb	/	Aromatic Solutions	185 € ⁵⁾	85 €
SENSORY FOUR SENSES							
SeS	Rank Order	907	Aug	Aug	4 Rank Order Sets (haptic and visual test, taste, odour)	372 € ⁵⁾	160 €
SENSORY ACCORDING TO DIN EN 22935; 1-3							
SeDLG1	Milk	879	Feb	Jan	Parameter according to DIN EN ISO 22935; 1-3 (5-point scale)	199 € ⁵⁾	80 €
SeDLG2	Dairy Products	912	Sep	Sep	Parameter according to DIN EN ISO 22935; 1-3 (5-point scale)	199 € ⁵⁾	80 €
SeDLG3	Powder	886	Mar	Mar	Baby foods and Milk Powder Parameter according to DIN EN ISO 22935; 1-3 (5-point scale)	199 € ⁵⁾	80 €
SENSORY FAT AND OIL							
SeO1	Virgin, cold pressed Rapeseed Oil	902	Jun	Jun	Parameter according to DGF-Einheits-Methode (fat)	195 € ⁵⁾	65 €
SeO2	Frying Fat	/	/	Nov	Parameter according to DGF-Einheits-Methode (fat)	195 € ⁵⁾	65 €
SENSORY DRINKING WATER							
SeTW	Drinking Water TON / TFN	899	May	May	Odour Threshold Value and Flavour Threshold Value in Drinking Water acc. to DIN EN 1622	352 € ⁴⁾	80 €

⁴⁾ Basic price contains **up to 3 panellists** already, the costs for additional test persons are only charged as of the 4th test person. **In any case**, please state how many panellists you would like to participate with before shipment!

⁵⁾ Basic price contains **one person**, any further person pay the price for additional panellists.

For Sensory-Proficiency Tests only:

If already known, please indicate the number of panellists in the field “message” when booking via online-portal, at latest please tell us when the announcement is sent!

Discount for Sensory Proficiency Testing Studies:

3 – 5 panellists: 5% discount ⁵⁾	6 – 9 panellists: 10% discount ^{4),5)}	as of 10 panellists = 15% discount ^{4),5)}
---	---	---



Please use our comprehensive services!



Accreditation
Provider of proficiency tests



Accreditation
Testing laboratory